



Health Solutions



HEELIFT
AFO Ultra



HEELIFT
Glide Ultra



HEELIFT
Classic



HEELIFT
Glide

HEELIFT
AFO



HEELIFT
Traction




HEELIFT® SUSPENSION BOOT
HEEL PROTECTOR



Instructions for Use (Note: Review cautions and warnings related to HEELIFT® device before selection and use.)

1. Determine appropriate size.

- Measure calf circumference. (see exhibit A.)
- Correlate the size of the calf circumference with the appropriate size of the HEELIFT® offloading boot on sizing chart and determine the proper size.
- Open the boot by undoing straps. (see exhibit B.)
- Set extra foam pad aside for optional customization. (Note: Customization should only be performed by your healthcare provider)
- Place foot in boot. (see exhibit C.)
- Place the lower extremity in the boot with the leg resting on the fixed elevation pad and the back of heel hanging off the fixed elevation pad over the heel opening so that no pressure is on heel. (see exhibit D.)

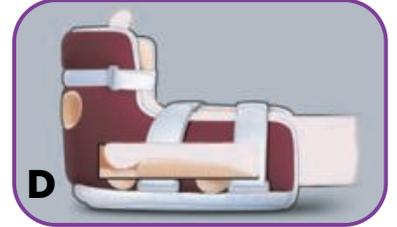

2. Secure the straps.

- Secure each strap. (see exhibit E.)
- Pull each strap over the foam pad of the boot over the leg and feed through the respective D-ring and then fasten the strap hook & loop closure back onto itself. (see exhibit E.)
- Start with the top strap and work your way downwards with each strap. (see exhibit E.)
- Straps should never be in contact with the skin. (see exhibit E.)
- Make sure each strap is fastened back onto itself with the hook & loop closure so that the hook & loop side of the strap is not exposed. (see exhibit F.)
- Use the Two-Finger Test to check to make sure each strap is fastened appropriately to ensure the boot is not too tight or not too loose and does not contact the skin. (see exhibit F.)



3. Check to make sure the heel is completely offloaded by:

- Lifting the leg and looking in the heel opening to ensure heel is completely offloaded and no pressure is on the back of the heel.(see exhibit G.)
- Put hand through heel opening and cup heel to ensure heel is completely offloaded and no pressure is on the back of the heel.(see exhibit H.)



1

4. Use of the Forefoot strap (**Note:** Use of forefoot strap should only be performed by your healthcare provider)

- The additional forefoot strap is only available on the Glide, Glide Ultra, AFO, and AFO Ultra HEELIFT® boot.
- The forefoot strap should only be used on people with good skin integrity.
- If not using the forefoot strap: Wrap strap around the underside of the boot, pull the strap through the D-ring, and secure the hook & loop to itself. (see exhibit I.)
- If using the forefoot strap: Secure the forefoot strap. (see exhibit J.)
- Pull the strap over the top of the forefoot portion of the boot and feed through its respective D-ring and secure the hook & loop strap to itself. (see exhibit J)
- The forefoot strap should never be in contact with the skin. (see exhibit J)
- Make sure each hook & loop strap is fastened back onto itself with the D-ring closure so that the hook & loop side is not exposed. (see exhibit J.)
- Use the Two-Finger Test to check to make sure each strap is fastened appropriately to ensure the boot is not too tight or not too loose and does not touch the skin. (see exhibit J.)



2

Indications for Use of HEELIFT® Classic, HEELIFT® Glide, HEELIFT® Glide Ultra, HEELIFT® AFO, and HEELIFT® Traction Boots.

For use on all heels with existing an existing pressure ulcer or a history of pressure ulcers at any location in the past. Use is also indicated for high-risk patients with two or three of the following clinical characteristics:

- Any person who is immobile or who has limited mobility who has an area at-risk for a pressure ulcer to develop on the foot or ankle.
- Any person who is immobile or who has limited mobility who has a preexisting pressure ulcer on their heel and/or ankle.
- Any person who has a Braden Score of less than or equal to 18 (<18).

3

Cautions

- The HEELIFT® offloading boot is a medical device used for the prevention and treatment of pressure ulcers. It should only be used under the guidance of your healthcare provider.
- A HEELIFT® offloading boot with a convoluted interior should only be used on a person with good skin integrity. If used on a person with poor skin integrity the convoluted texture can lead to compromise of the skin.
- Make sure the HEELIFT® boot is of the appropriate size before applying. Always measure the calf circumference and correlate the measurement of the calf circumference to the sizing chart to determine the appropriate size of the HEELIFT® boot.
- Note: It is important to determine the appropriate size of the HEELIFT® boot for each individual person so that the boot is not too small causing pressure on the skin leading to a pressure ulcer and so that the boot is not too loose causing shear and friction forces on the skin leading to a pressure ulcer.
- Make sure straps never touches the skin to not cause pressure, shear, or forces on the skin which could cause a pressure ulcer.
- Use the 2-finger test after securing the straps to make sure the boot is not too tight or too loose.
- The HEELIFT® offloading boot is a single patient only – limited multiple use medical device.

4 Warning

- All customization of the HEELIFT® boot should only be performed by the healthcare provider. If the boot is not customized appropriately to properly offload an at-risk area or area of pre-existing wound undue pressure can occur on the skin therefore leading to development of a pressure ulcer or worsening of a pre-existing wound.
- Forefoot strap on HEELIFT® Glide boot is only recommended for people with good skin integrity. If used on a person with poor skin integrity can cause pressure or shear and friction force on underlying skin resulting in a pressure ulcer. Please seek opinion of healthcare provider before using.
- The leg should never move within the boot. If the leg moves within the boot, the boot is not applied appropriately and injury to the skin from shear and friction forces against the skin from the boot can cause injury to the skin.
- Make sure adhesive side of extra foam pad never touches the skin to avoid any reaction from the adhesive on the skin, or any compromise of the skin from the adhesive.
- SCD tubing should always carefully be placed into the groove built into the boot so that it never touches the skin, to avoid compromise of the skin from the tubing.
- Ventilation holes are meant for air circulation within the boot. Do not place any tubing through the ventilation holes in the boot.
- As per standard of care, remove HEELIFT® boot and inspect skin every 8 hours to ensure no compromise of the skin has occurred.
- Discontinue the HEELIFT® offloading boot if you experience any pain, compromise of the skin or skin break down, redness or other changes in skin color, abnormal swelling, or other issue while wearing the boot and contact your healthcare provider immediately or go to your nearest emergency room for immediate care and attention.

5 Customization (Note: Customization should only be performed by your healthcare provider. If using the HEELIFT® Ultra boots pull back the removable elevation cover first.)

The HEELIFT® offloading boot can be customized to offload other at-risk areas in addition to the back of the heel including the Achilles Tendon, Malleolar Decubitus, Foot Drop, hip and/or foot rotation, and SCD Tubing.

1. Achilles Tendon. (see exhibit K)

- Make an upside-down V cut or an upside-down U cut as determined appropriate by your healthcare provider in the bottom of the fixed elevation pad to appropriately offload the Achilles tendon.



2. Malleoli (ankle bones) (see exhibit L)

- Make an oblique cut or an upside-down hockey stick cut as determined appropriate by your healthcare provider on the side of the elevation pad starting from a point just above the ankle bone and cutting downward through the bottom of the fixed elevation pad so that the ankle bone is completely offloaded.
- If further offloading is required as determined by your healthcare provider place the extra foam pad in the groove on the side of the ankle bone needing to be offloaded with the bottom of the pad just above the ankle bone and cut the top of the extra foam pad flush with the top of the boot. Attach the extra foam pad to the side of the boot once appropriately positioned in the groove by peeling the adhesive backing off the extra foam pad. Make sure the adhesive side never touches the skin.



3. Foot Drop (see exhibit M)

- Measure the extra foam pad from the tip of the toes to the area where the arch meets the heel.
- Cut the extra foam pad at the area where the arch meets the heel and bevel the edge.
- Peel the adhesive backing off the extra foam pad.
- Position the extra foam pad vertically under the patient's foot so that the beveled edge is under the area where the arch meets the heel, and the adhesive side of the pad, is against the bottom of the boot to not touch the skin (make sure adhesive never touches the skin).



4. Hip and/or Foot Rotation (see exhibit N.)

- Use the optional Anti-Rotation Wedge to prevent hip and/or foot rotation. See instructions included with the wedge.
- The Anti-Rotation Wedge gives you the flexibility needed to stop rotation in immobile patients. The easy to apply, reusable wedge attaches to either side of the boot, and prevents rotation.
- Works for both external and internal rotation.



5. SCD Tubing Placement (see exhibit O)

- Place SCD tubing in the groove built into the boot along the side of the boot, between the elevation pad and the side of the boot opposite the side with the attached D-rings. This allows the tubing to lay flat and to exit the boot without touching the skin.
- SCD tubing should always carefully be placed into the groove, built into the boot, so that it never touches the skin to avoid compromise of the skin from the tubing.
- Ventilation holes are meant for air circulation within the boot. Do not place any tubing through the ventilation holes in the boot.



6

Technical Data

Contents of Package

- HEELIFT® offloading boot
- Single patient-Multiple use
- Extra foam pad for optional customization of boot (should only be performed by your healthcare provider)
- Instructions for use
- Anti-Rotation Wedges (optional)
 - HEELIFT® Ultra models include an Anti-Rotation Wedge

Size: Calf Circumference

- Petite: 15-25 cm (6-10 inches)
- Standard: 25-38 cm (10-15 inches)
- Bariatric: 38-58 cm (15-23 inches)

Interior

- Smooth
- Convoluted (should only be used by people with good skin integrity and without comorbidity)
- Ultra (lined with water repellent liner indicated for draining wounds)



7

Cleaning (Caution: Clean or disinfect using a nonbleach gentle detergent or a nonbleach disinfectant. As with any medical device, bleach can breakdown the integrity of the material of the HEELIFT® offloading boot. To maintain the integrity of the HEELIFT® we recommend sanitizing or hand washing.)

1. To sanitize

- Use a nonbleach disinfectant wipe or spray.

2. To hand wash

- Wash in warm water with a mild nonbleach detergent.

3. To machine wash and dry

- Secure all straps.
- Remove traction device if using HEELIFT® traction boot.
- Place in mesh HEELIFT® brand, regular mesh laundry bag, or pillowcase.
- Machine wash in warm water (40°-60°C/105°-140°F) gentle cycle with a mild nonbleach detergent.
- Machine dry on low heat.

Instructions for Traction Boot (Note: Review indications, cautions, and warnings related to HEELIFT® device before use.)

- PRE-OPERATIVE - the HEELIFT® Traction Boot for extension helps to stabilize femur fractures prior to surgery and enables to apply straight skin traction with up to 4.5 kg/ 10 lbs. (Buck's traction).
- POST-OPERATIVE - without traction device mechanism converts to suspension boot to aid in the prevention of pressure injuries/ulcers during rehabilitation.

PRE-OPERATIVE


A. Application of the suspension boot

- Open the HEELIFT® Traction Boot. Remove the spare foam pad. Please keep the spare pad available; see optional customization instructions.
- Place the patient's foot into the extension boot and ensure that the heel is positioned directly above the heel suspension opening. The heel should hang over the bottom elevation pad. See photo 1.
- For closing pull the hook & loop fastener straps over the leg towards the D-rings. Thread the straps through the D-rings. Use the hook & loop fastener closures to secure the straps. See photo 2.
- Test for the proper fit by trying to remove the closed extension boot. Test the fit under straps and heel opening using the "Two-Finger" test. See photo 3. The boot should not be placed neither too loose nor too tight around the leg. The hook & loop fastener straps should not be in contact with the skin.
- To prevent rotation of the foot use the Anti-Rotation Wedge (available separately) and place it on the left or right side along with the tibia.
- To prevent foot drop, see Section 5 for customization instructions.



B. Application of traction device

- Remove the long hook & loop fastener attached traction straps (D) from the sides of the traction boot.
- Unravel the traction rope (A) and double knot one end to the rope attachment bar (B).
- Fix the rope attachment bar with the hook & loop fastener traction straps to both sides of the HEELIFT® Traction Boot. Place the plate for the traction bar to be outside.
- Pass the unknotted end of the traction rope through the prepositioned traction pulley on the cross bar attached to the frame at the foot of the bed.
- Pull firmly on the rope and create a short 2.5 cm (1-inch) large loop in the rope and secure with the appropriate knot (not a slip knot) just beyond the pulley.
- Attach a weight hanger with the prescribed weight (max. 4.5 kg/10 lbs.).
- Elevate the extension boot together with the traction bar so that the HEELIFT® Traction Boot and the leg are 0.6 cm (0.24 in) above the bed. You should be able to fit your finger between the heel opening and the bed.
- If the leg is externally rotated, apply the Anti-Rotation Wedge (available separately) beneath the traction straps on the outside of the traction boot.
- To avoid foot drop, secure the extra pad in a vertical position behind the sole of the foot. see Section 5 for customization instructions.

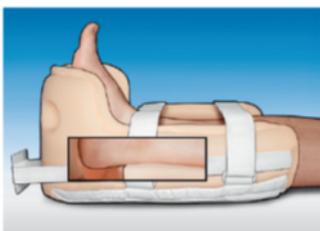

POST-OPERATIVE

A. Convert HEELIFT Traction boot to suspension boot

1. Remove the side traction straps, traction bar and rope.
2. Follow application instructions, pre-operative number 1 to 5.
3. Follow customization instructions for the spare foam pad (see Section 5 - Customization).

Intended Use Statement

HEELIFT® Traction boot is a medical device used for stabilizing fractures prior (pre-operative) to surgery (resembling Bucks Traction) and provides leg elevation after surgery (post-operative) to prevent pressure injuries/ulcers.

Indications

- **Pre-operative** for preparing the extension or
- **Post-operative** for prevention of pressure injuries/ulcers
- Disease or condition:
 - Patients with lower extremity fractures
 - Post-operative patient requiring elevation
 - Patients at risk for pressure injuries/ulcers
 - Patients with fracture and pain
 - Patients with displaced fracture

Contraindications

- Open fractures
- Bleeding wounds
- Elderly patients' skin is fragile and may be injured from the traction
- Osteoporosis

Cautions

- Make sure top of the HEELIFT® Traction boot is below fibular lead.
- The HEELIFT® Traction Boot for extension is only designed for the use with bedridden patients and intended for inpatient use.
- In case of improper handling, the function and maximum safety of the product can no longer be guaranteed.
- This aid is intended for single patient – multiple use only.

Warnings

- The HEELIFT® Traction boot should be removed every 8 hours to inspect skin.
- Do not use over open wounds; the HEELIFT® Traction Boot is to be used on patients with intact skin only.
- Do not use this device if it was damaged and/or packaging has been opened.
- All customization of the HEELIFT® boot should only be performed by the healthcare provider. If the boot is not customized appropriately to properly offload an at-risk area or area of pre-existing wound undue pressure can occur on the skin therefore leading to development of a pressure ulcer or worsening of a pre-existing wound.
- The leg should never move within the boot. If the leg moves within the boot, the boot is not applied appropriately and injury to the skin from sheer and friction forces against the skin from the boot can cause injury to the skin.
- Make sure adhesive side of extra foam pad never touches the skin to avoid any reaction from the adhesive on the skin, or any compromise of the skin from the adhesive.
- SCD tubing should always carefully be placed into the groove built into the boot so that it never touches the skin, to avoid compromise of the skin from the tubing.
- Ventilation holes are meant for air circulation within the boot. Do not place any tubing through the ventilation holes in the boot.

- Discontinue the HEELIFT® Traction boot if you experience any pain, compromise of the skin or skin break down, redness or other changes in skin color, abnormal swelling, or other issue while wearing the boot and contact your healthcare provider immediately or go to your nearest emergency room for immediate care and attention.
- If you develop an allergic reaction and/or experience itchy, red skin after coming into contact with any part of this device, please stop using it and contact your healthcare professional immediately.

Technical Data

Contents of Package

- HEELIFT® Traction offloading boot
- Traction metal bar with nylon hook-and-loop fastener
- Traction nylon rope
- Extra foam pad
- Anti-Rotation Wedges (optional)
- Application and Fit Instructions

Size: Calf Circumference

Standard: 25-38cm (10-15 inches)

Color:

Beige

Interior:

Smooth

Maintenance:

The product does not require maintenance.




Cleaning Instructions

- **Cleaning:** Remove traction device before cleaning.
To hand wash: Use non-bleach, mild cleaner and warm water.
- **To machine wash and dry:** Secure straps and place in net laundry bag or pillowcase. Wash with mild detergent (40°-60°C/105°-140°F), do not use bleach, and dry on low temperature. Allow to dry completely before reapplying boot to patient.
- **To sanitize:** Wipe with sanitizing wipes or spray, dry completely before using.

Anti-Rotation Wedge:



- See instructional Diagram 1 for use of the Anti-Rotation Wedge with the Suspension Boot.

LEFT LEG

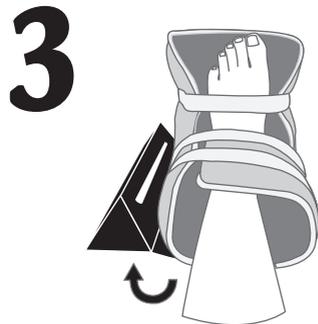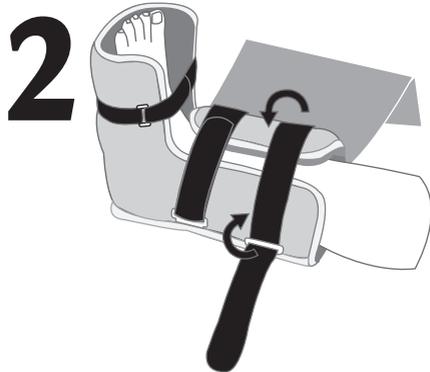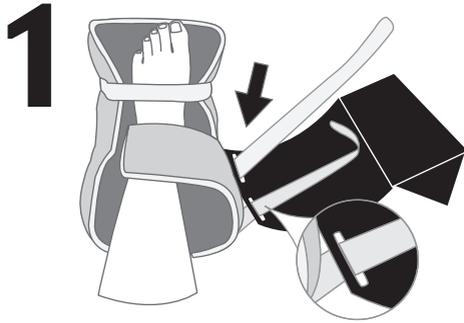

RIGHT LEG

Diagram 1

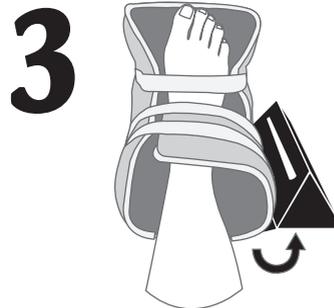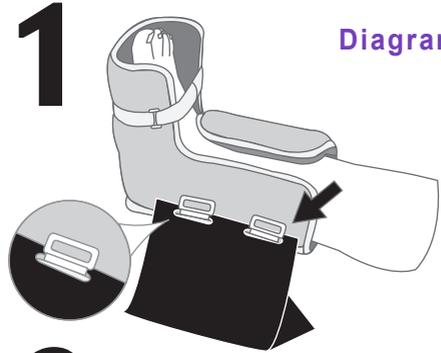



Consult Instructions for Use



EN-ENGLISH



ES-ESPAÑOL



DE-DEUTSCH



DA-DANSK



FR-FRANÇAIS



IT-ITALIANO



LT-LIETUVŲ KALBA



NL-DUTCH



NO-NORSK



PL-POLSKI



PT-PORTUGUÊS



PT-B PORTUGUÊS BRASIL



RO-ROMÂNĂ



SK-SLOVENSKÝ JAZYK



SL-SLOVENŠČINA



SV-SVENSKA



TL-TAGALOG

TR-TÜRKÇE



Walgreen Health Solutions, LLC
1316 Sherman Avenue
Evanston, IL 60201
Phone: (847) 328-9540
Email: info@walgreenhealthsolutions.com
www.walgreenhealthsolutions.com Made in China

CH

REP

EC

REP

MedEnvoy
Prinses Margrietplantsoen 33 - Suite 123
2595 AM The Hague
The Netherlands

Emergo Europe B.V
Prinsessegracht 20
2514 AP The Hague
The Netherlands



Heel Protector

ES	Protector de talón
DE	Fersenschutz
DA	Hælbeskytter
FR	Protecteur de talon
IT	Protezione del tallone
LT	Kulno gynėjas
NL	Hielbeschermer
NO	Hælbeskytter
PL	Ochraniacz pięty
PT	Protetor de calcanhar
PT-B	Protetor de calcanhar
RO	Protector pentru toc
SV	Hälskydd
SK	Chráníč päty
SL	Ščitnik pete
TL	Protektor sa takong
TR	Cok koruyucu

Suspension Boot

ES	Bota de suspension
DE	Freilagerungstiefel
DA	Affjæring støvle
FR	Botte de suspension
IT	Stivale di sospensione
LT	Pakabos bagažinė
NL	Verende laars
NO	Fjæring støvel
PL	Bagażnik zawieszania
PT	Bota de Suspensão
PT-B	Bota de suspensão
RO	Cizmă suspendată
SV	Upphängnings stövel
SK	Zavesenie topánok
SL	Vzmetni prtljažnik
TL	Pagkatigil bota
TR	Süspansiyonlu çizme

ANTI-ROTATIONAL WEDGE ONLY (INCLUDED WITH AFO ULTRA AND GLIDE ULTRA)

Anti-Rotation Wedge

ES	Cuña antirrotación
DE	Anti-Rotations-Keil
DA	Anti-rotations kile
FR	Coin anti-rotation
IT	Cuneo antirotazione
LT	Anti-sukimosi pleištas
NL	Anti-rotatie wig
NO	Antirotasjonskile
PL	Klin antyobrotowy
PT	Cunha Anti-rotação
PT-B	Cunha Anti-Rotação
RO	Pană anti-rotăție
SV	Antirotationskil
SK	Protirotačný klin
SL	Protirotačijski klin
TL	Anti rotation dila
TR	Dönme önleyici kama

Freestanding Patient Positioner, Reusable

ES	Posicionador de paciente independiente, reutilizable
DE	Autonomer Patienten Positionierer, wiederverwendbar
DA	Fritstående patientpositioner, genanvendelig
FR	Positionneur de patient autonome, réutilisable
IT	Posizionatore paziente indipendente, riutilizzabile
LT	Laisvai pastatomas paciento padėties įtaisas, daugkartinis
NL	Vrijstaande patiëntversteller, herbruikbaar
NO	Frittstående pasientposisjoner, gjenbrukbar
PL	Wolnostojący pozycjoner pacjenta, wielokrotnego użytku
PT	Posicionador autónomo do paciente, reutilizável
PT-B	Posicionador autónomo do paciente, reutilizável
RO	Poziționator independent pentru pacient, reutilizabil
SV	Fristående patientpositioner, återanvändbar
SK	Voľne stojace polohovadlo pacienta, opakovane použiteľné
SL	Samostoječi pozicioner za paciente, za večkratno uporabo
TL	Freestanding positioner reusable pasyente
TR	Bağımsız Hasta Konumlandırıcı, Yeniden Kullanılabilir



Single Patient - Multiple Use

ES	Paciente único - Uso múltiple
DE	Einzelpatient – Mehrfachverwendung
DA	Enkelt patient - flergangsbrug
FR	Patient unique - Usage multiple
IT	Singolo paziente - Uso multiplo
LT	Vienas pacientas – daugkartinis naudojimas
NL	Eén patiënt - meervoudig gebruik
NO	Enkelt pasient - Flerbruk
PL	Jeden pacjent — wiele zastosowań
PT	Paciente Único - Uso Múltiplo
PT-B	Paciente único - Uso múltiplo
RO	Pacient unic - Utilizare multiplă
SV	Enstaka patient - Flera användningsområden
SK	Jeden pacient – viacnásobné použitie
SL	En bolnik - večkratna uporaba
TL	bawat pasyente - ng iba
TR	Tek Hasta - Çoklu Kullanım



Consult Instructions for Use

ES	Consultar instrucciones de uso
DE	Lesen Sie die Gebrauchsanweisung
DA	Se brugsanvisningen
FR	Consulter les instructions d'utilisation
IT	Consultare le istruzioni per l'uso
LT	Pasikonsultuokite naudoti naudojimą instrukcijas
NL	Raadpleeg de instructies voor gebruik
NO	Kontakt instruksjonene for bruk
PL	Skonsultuj się z instrukcjami do użycia
PT	Consulte as instruções de uso
PT-B	Consulte as instruções de uso
RO	Consultați instrucțiunile de utilizare
SV	Konsultera bruksanvisningen
SK	Konzultujte pokyny na použitie
SL	Oglejte si navodila za uporabo
TL	Sasangguni tagubilin gamitin
TR	Kullanım için talimatlara danışın



Unique Device Identifier

ES	Identificador de dispositivo único
DE	Eindeutige Geräteerkennung
DA	Unikt enheds Identifikator
FR	Identifiant unique de l'appareil
IT	Identificatore univoco del dispositivo
LT	Unikalus įrenginio identifikatorius
NL	Unieke apparaatindicator
NO	Unik enhetsidentifikator
PL	Unikalny identyfikator urządzenia
PT	Identificador Único de Dispositivo
PT-B	Indicador único de dispositivo
RO	Identificator unic de dispozitiv
SV	Unik enhetsidentifierare
SK	Jedinečný identifikátor zariadenia
SL	Edinstven indikator naprave
TL	Tulali banta identifier
TR	Benzersiz Cihaz Tanımlayıcı



Latex-Free (Not Made with Natural Rubber Latex)

ES	Sin látex
DE	Latexfrei
DA	Latex fri
FR	Sans latex
IT	Senza latex
LT	Be latekso
NL	Latex vrij
NO	Uten latex
PL	Bez lateksu
PT	Látex grátis
PT-B	Sem látex
RO	Fără latex
SV	Latex fri
SK	Bez latexu
SL	Brez lateksa
TL	Walang Latex
TR	Lateks içermez

MD Medical Device

ES	Dispositivo médico
DE	Medizinprodukt
DA	Medicinsk udstyr
FR	Dispositif médical
IT	Dispositivo medico
LT	Medicininis prietaisas
NL	Medisch apparaat
NO	Medisinsk enhet
PL	Urządzenie medyczne
PT	Aparelho médico
PT-B	Aparelho médico
RO	Aparat medical
SV	Medicinsk utrustning
SK	Lekárska pomôcka
SL	Medicinski pripomoček
TL	Gamit Medikal
TR	Tıbbi cihaz

**Importer**

ES	Importador
DE	Importeur
DA	Importør
FR	Importateur
IT	Importatore
LT	Importuotojas
NL	Importeur
NO	Importør
PL	Importer
PT	Importador
PT-B	Importador
RO	Importator
SV	Importör
SK	Dovozca
SL	Uvoznik
TL	Mang-aangkat
TR	İthalatçı

**Keep Dry and Away from Direct Sunlight**

ES	Manténgase seco y alejado de la luz solar directa
DE	Trocken lagern und vor direkter Sonneneinstrahlung schützen
DA	Hold dig tør og væk fra direkte sollys
FR	Garder sèche et loin de la lumière directe du soleil
IT	Mantieniti asciutto e lontano dalla luce solare diretta
LT	Laikykite sausas ir toli nuo tiesioginių saulės spindulių
NL	Droog en uit de buurt van direct zonlicht houden
NO	Hold deg tørr og vekk fra direkte sollys
PL	Przechowywać w suchym miejscu i z dala od bezpośredniego światła słonecznego
PT	Mantenha seco e longe da luz solar direta
PT-B	Manter seco e afastado da luz direta do sol
RO	Păstrați uscare și departe de lumina directă a soarelui
SV	Håll torr och bort från direkt solljus
SK	Uchovávať v suchu a mimo dosahu priameho slnečného svetla
SL	Hranite suho in stran od neposredne sončne svetlobe
TL	At ang tuyong ang magtuturo sa sunlight
TR	Kuru ve doğrudan güneş ışığından uzak durun